


**SpiderFX<sup>®</sup>**

Embolic Protection Device

*Filter* the risk<sup>™</sup>

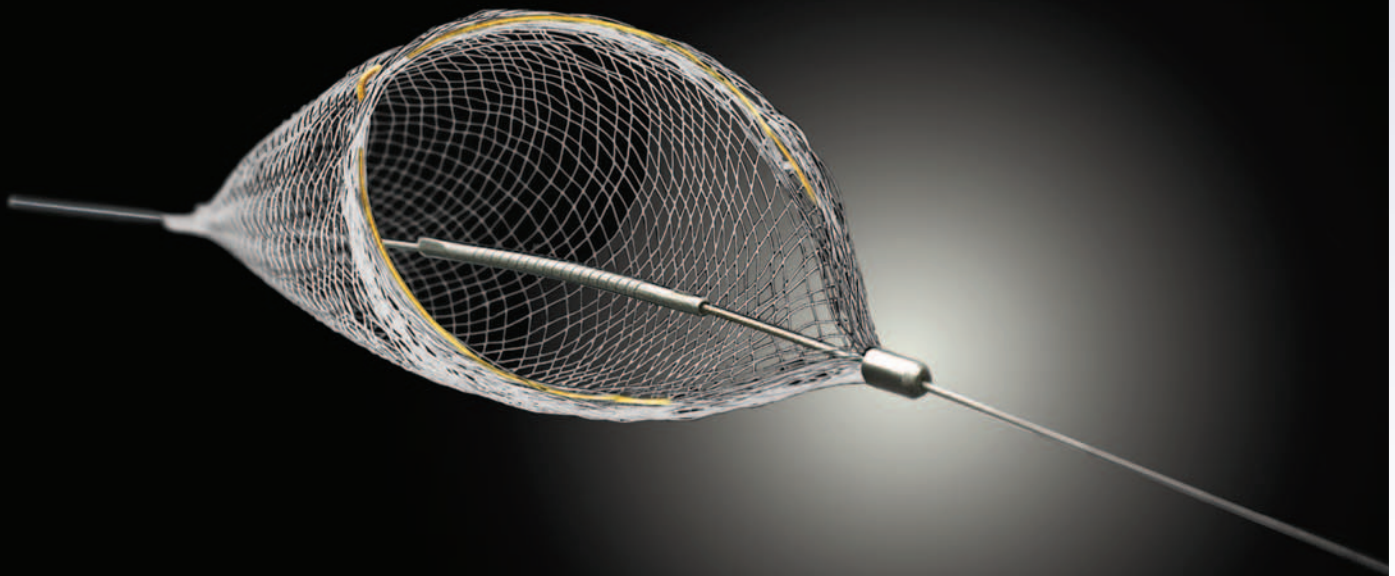

For the ultimate in embolic  
protection.

# Designed to deliver the ideal balance of blood flow and debris capture.

SpiderFX® Embolic Protection Device

---


## Guidewire of Choice

- Works with any 0.014" or 0.018" guidewire to cross the most challenging carotid lesions




## Extensive Portfolio

- Treat vessels from 3 mm to 7 mm with a variety of sizes; available for both Carotid and SVG interventions

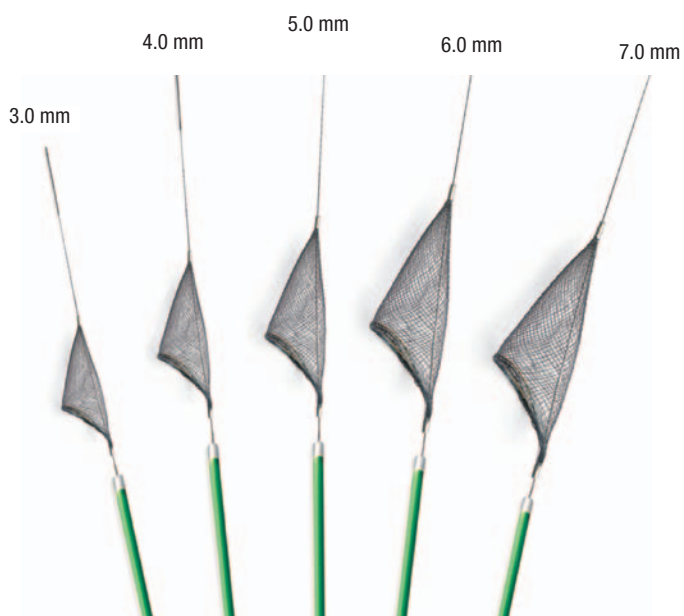

## Enhanced Visibility

- Clearly visible radiopaque markers and direct mouth indicator enable quick and controlled positioning of the filter throughout the intervention

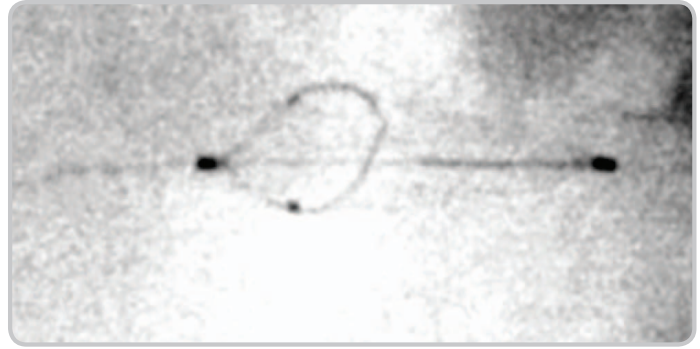

---

## Excellent Stability

- Controlled filter positioning throughout the intervention and during device exchanges
  - Braided nitinol design provides full-wall apposition
  - Capture wire designed to rotate and move longitudinally independent of the filter



# SpiderFX® Embolic Protection Device

COMPONENT			CAPTURE WIRE		DELIVERY END	RECOVERY END	GUIDE CATHETER/SHEATH
Model Number	Filter Size (mm)	Lumen Size (mm)	Wire Length OTW/RX (cm)	Wire Diameter (in/mm)	Crossing Profile (F)	Diameter (F)	Minimum ID (in)
SPD2-US-030-190	3.0	3.0	190	0.014/0.36	3.2	4.2	0.066
SPD2-US-030-320	3.0	3.0	320/190	0.014/0.36	3.2	4.2	0.066
SPD2-US-040-190	4.0	3.1-4.0	190	0.014/0.36	3.2	4.2	0.066
SPD2-US-040-320	4.0	3.1-4.0	320/190	0.014/0.36	3.2	4.2	0.066
SPD2-US-050-190	5.0	4.1-5.0	190	0.014/0.36	3.2	4.2	0.066
SPD2-US-050-320	5.0	4.1-5.0	320/190	0.014/0.36	3.2	4.2	0.066
SPD2-US-060-190	6.0	4.5-6.0	190	0.014/0.36	3.2	4.2	0.066
SPD2-US-060-320	6.0	4.5-6.0	320/190	0.014/0.36	3.2	4.2	0.066
SPD2-US-070-190	7.0	5.5-6.0 SVG 5.5-7.0 Carotid	190	0.014/0.36	3.2	4.2	0.066
SPD2-US-070-320	7.0	5.5-6.0 SVG 5.5-7.0 Carotid	320/190	0.014/0.36	3.2	4.2	0.066

The SpiderFX Embolic Protection Device allows the use of any 0.014" - 0.018" guidewire. The SpiderFX Embolic Protection Device is delivered in a single hoop, with Capture Wire/Filter pre-loaded in the Delivery End of the SpiderFX Catheter. The SpiderFX Embolic Protection Device is compatible with a guide catheter/sheath minimum ID of 0.066" (typically a 6F guide catheter or 5F access/long sheath). Check catheter manufacturer information for size and compatibility.

Indications, contraindications, warnings and instructions for use can be found in the product labeling supplied with each device.

**CAUTION:** Federal (USA) law restricts this device to sale by or on the order of a physician.

**Carotid Indication:** The SpiderFX Embolic Protection Device is indicated for use as a guidewire and embolic protection system to contain and remove embolic material (thrombus/debris) while performing angioplasty and stenting procedures in carotid arteries. The diameter of the artery at the site of the filter basket placement should be between 3.0 mm and 7.0 mm.

**SVG Indication:** The SpiderFX Embolic Protection Device is indicated for use as an embolic protection system to contain and remove embolic material (thrombus/debris). The device also acts as the guidewire while performing percutaneous transluminal coronary angioplasty or stenting procedures in coronary saphenous vein bypass grafts with reference vessel diameters of 3.0 to 6.0 mm. The safety and effectiveness of this device as an embolic protection system have not been established in the cerebral and peripheral vasculature.

## NEUROVASCULAR | PERIPHERAL VASCULAR

Access · Balloons · Embolic Coils · Embolic Protection · Liquid Embolics · Plaque Excision · Procedural Support · Retrieval Device · Stents

### ev3 Corporate

#### World Headquarters

#### Peripheral Vascular

9600 54th Avenue North  
Plymouth, MN 55442-2111  
USA

PH +1 763 398 7000

FX +1 763 398 7001

Cust Serv +1 800 716 6700

www.ev3.net

### ev3 Neurovascular

9775 Toledo Way  
Irvine, CA 92618  
USA

PH +1 949 837 3700

FX +1 949 837 2044

### ev3 Europe

#### International Headquarters

106-108 rue La Boétie  
75008 Paris  
France

PH +33 156 88 59 10

FX +33 156 88 59 11

